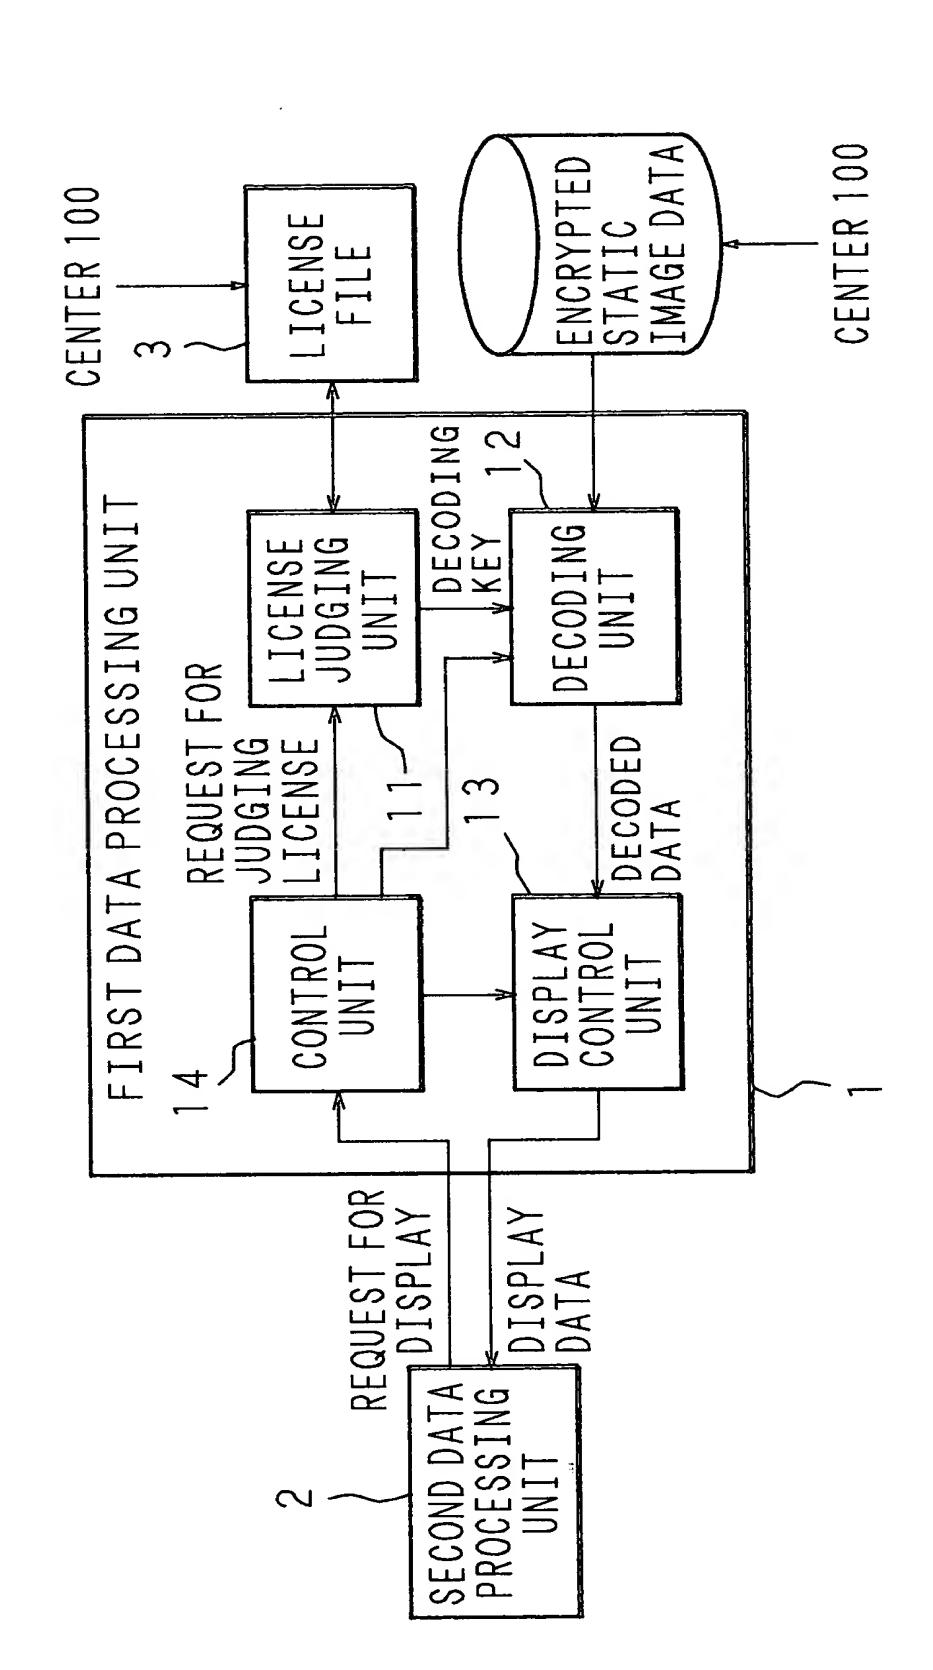


FIG. 2





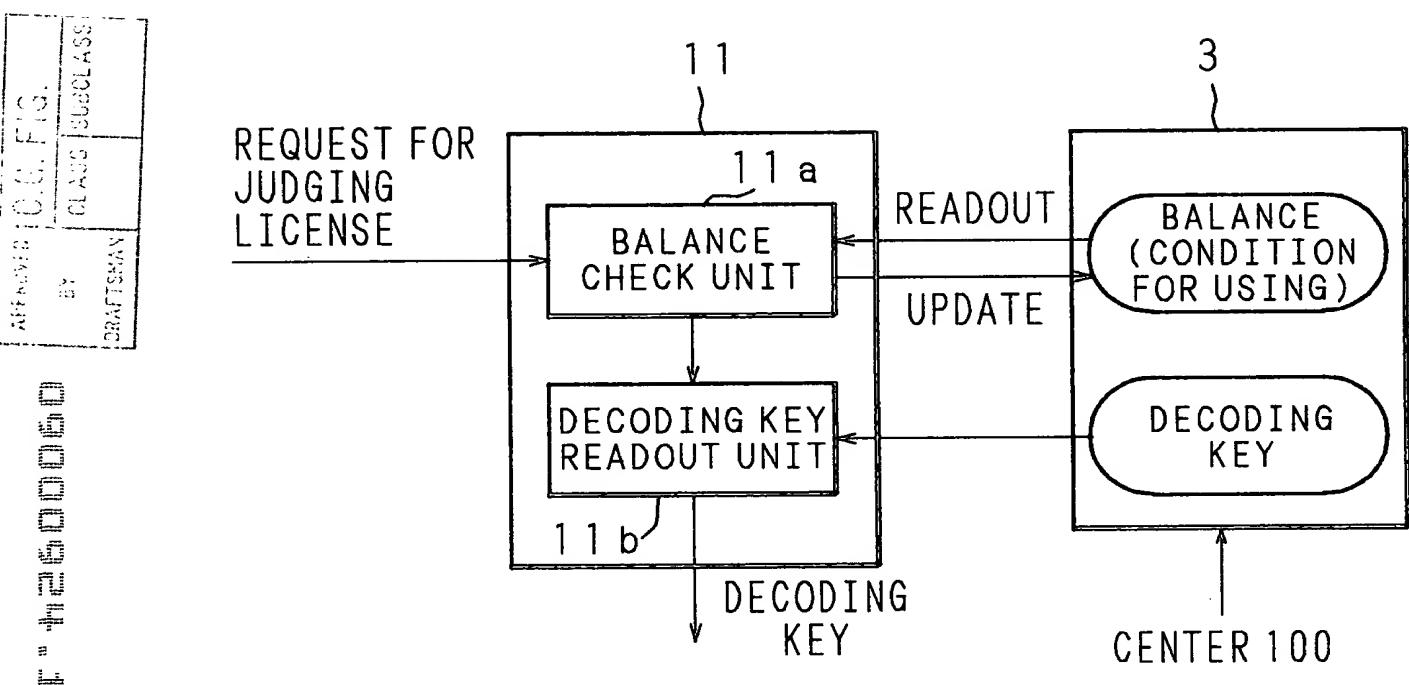


FIG. 4

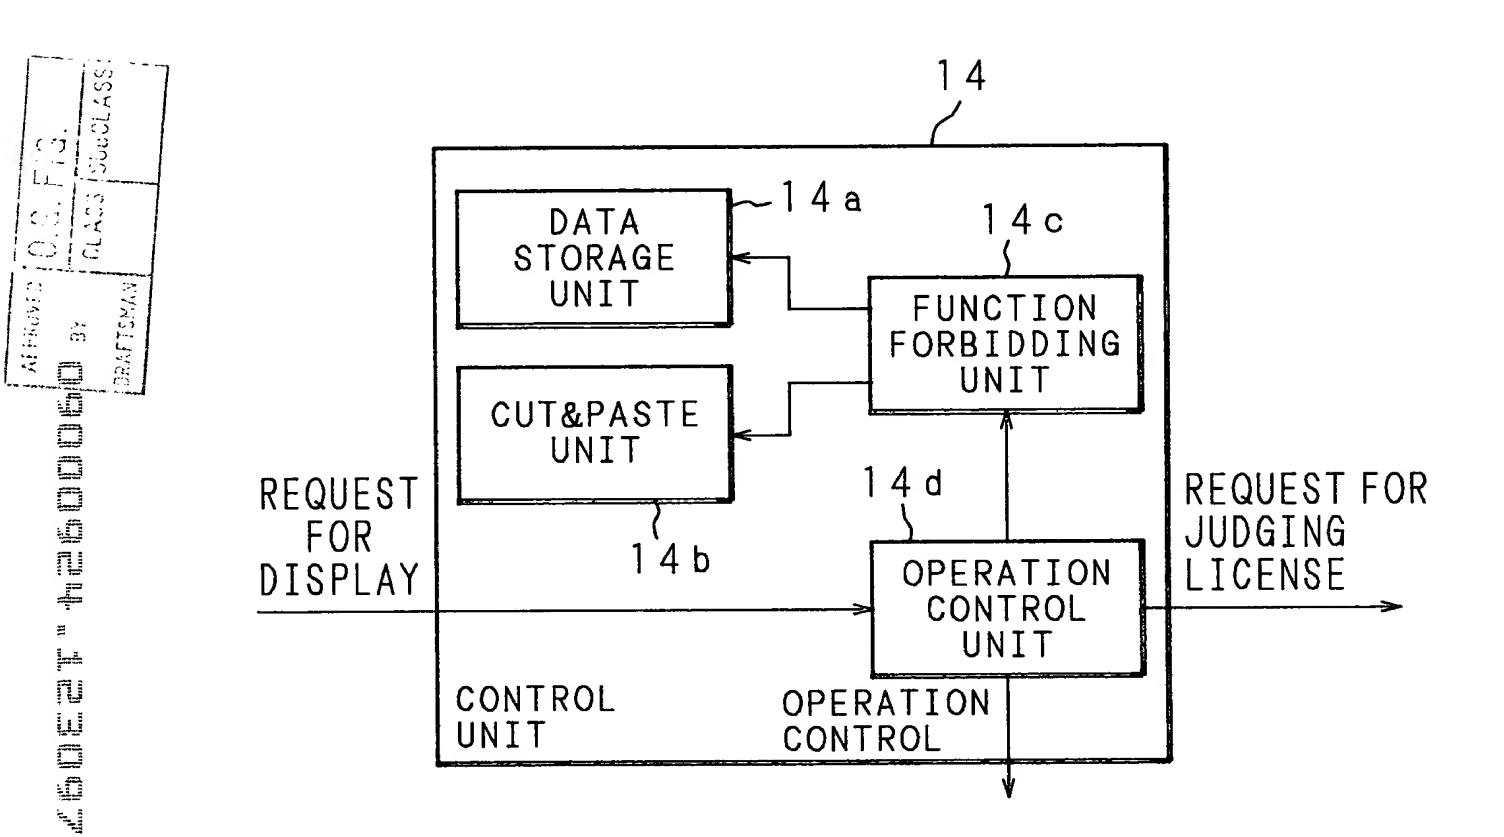


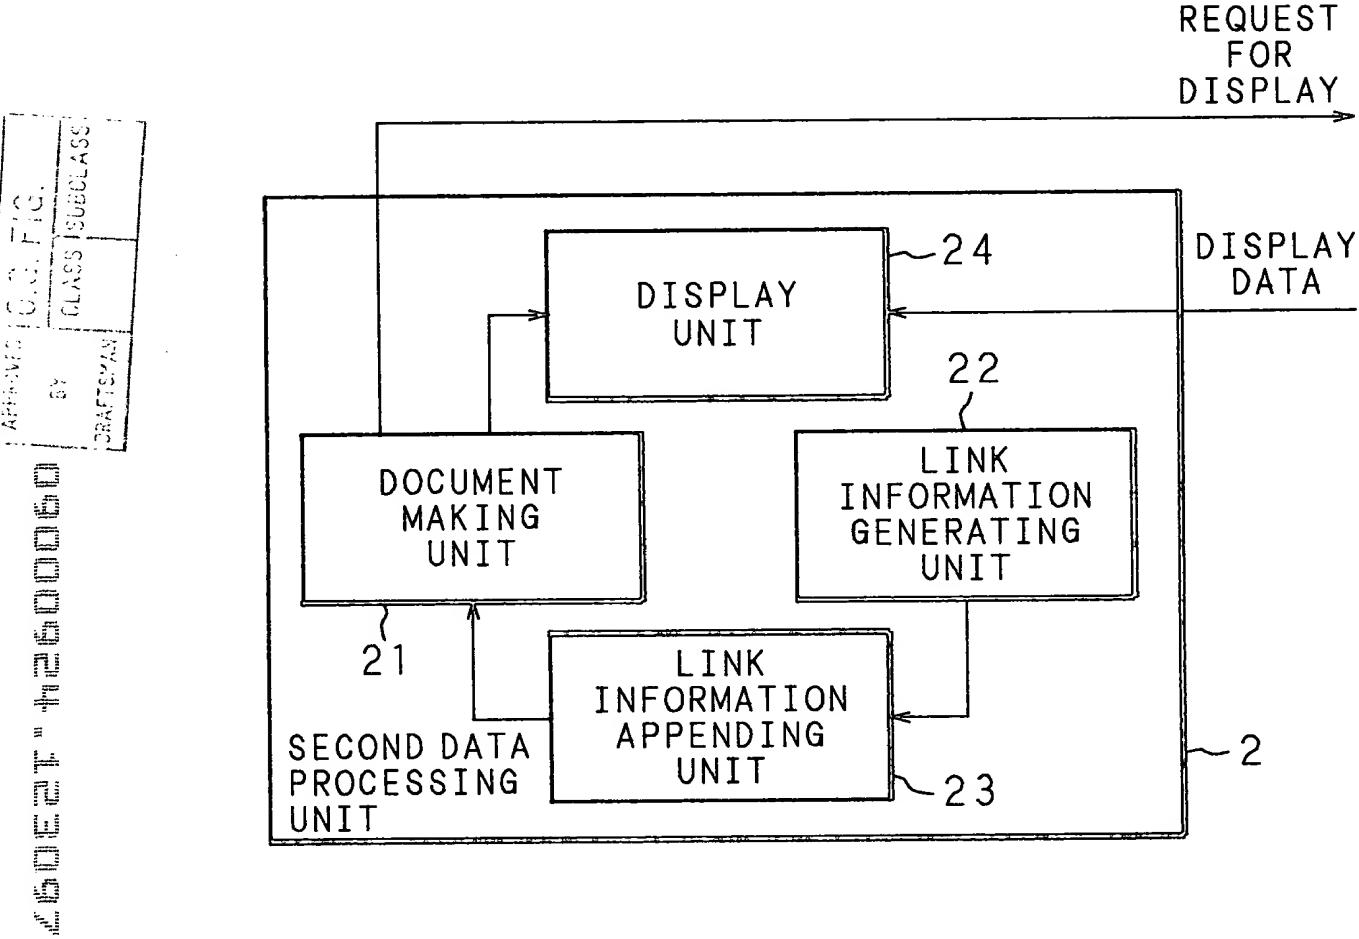

Airenvi

CAMPICAAN

FIG. 6

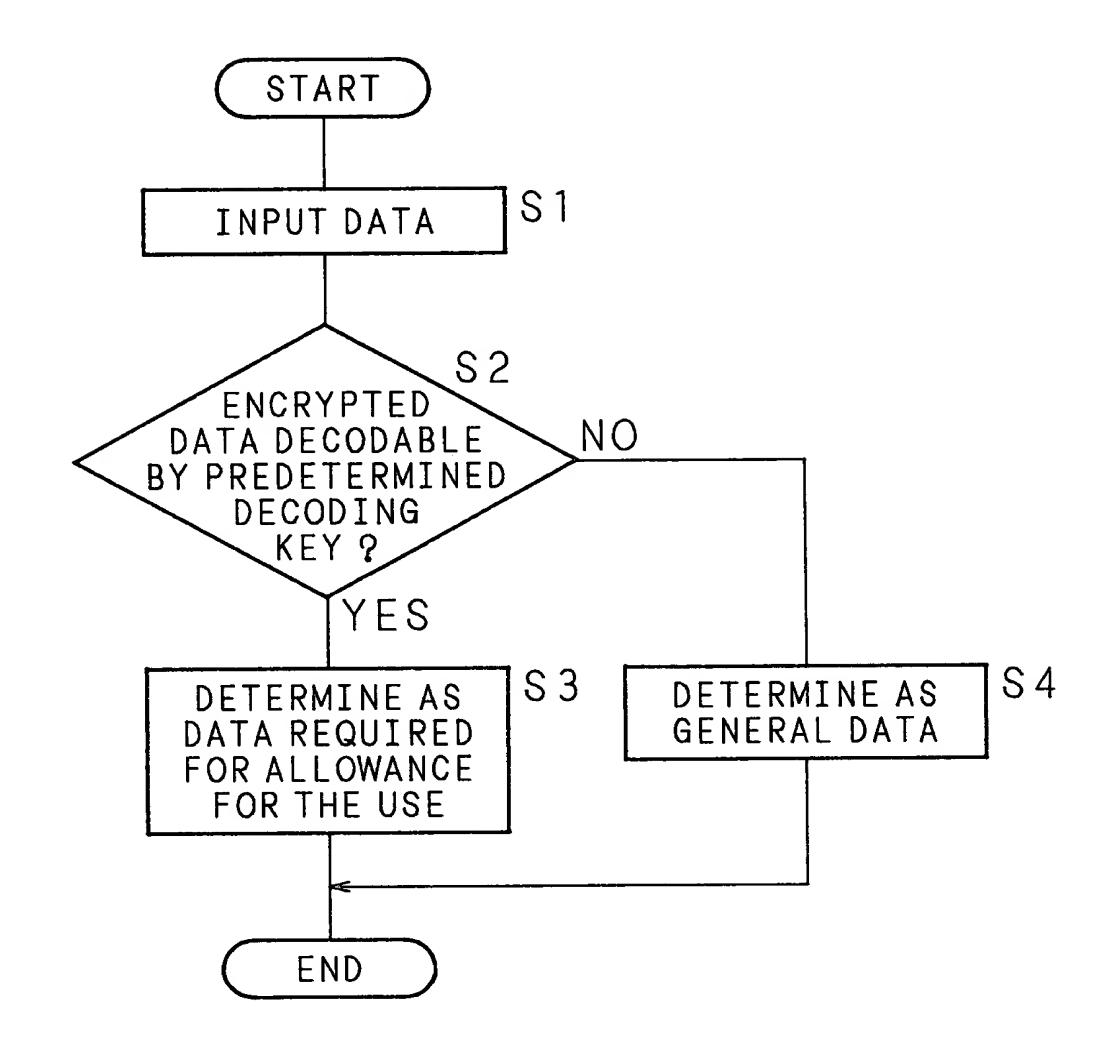

AFFECTION OF C. C. S. S. C. C. ASC.

FIG. 7

1		\cap	\cap		1 k /	N	T
	<i>)</i>	U	U	U	ΙV	IV	ı

Pleased to	meet you, · · ·
• • • •	
	STATIC IMAGE REQUIRED FOR
	ALLOWANCE FOR
	THE USE

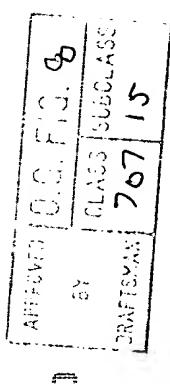
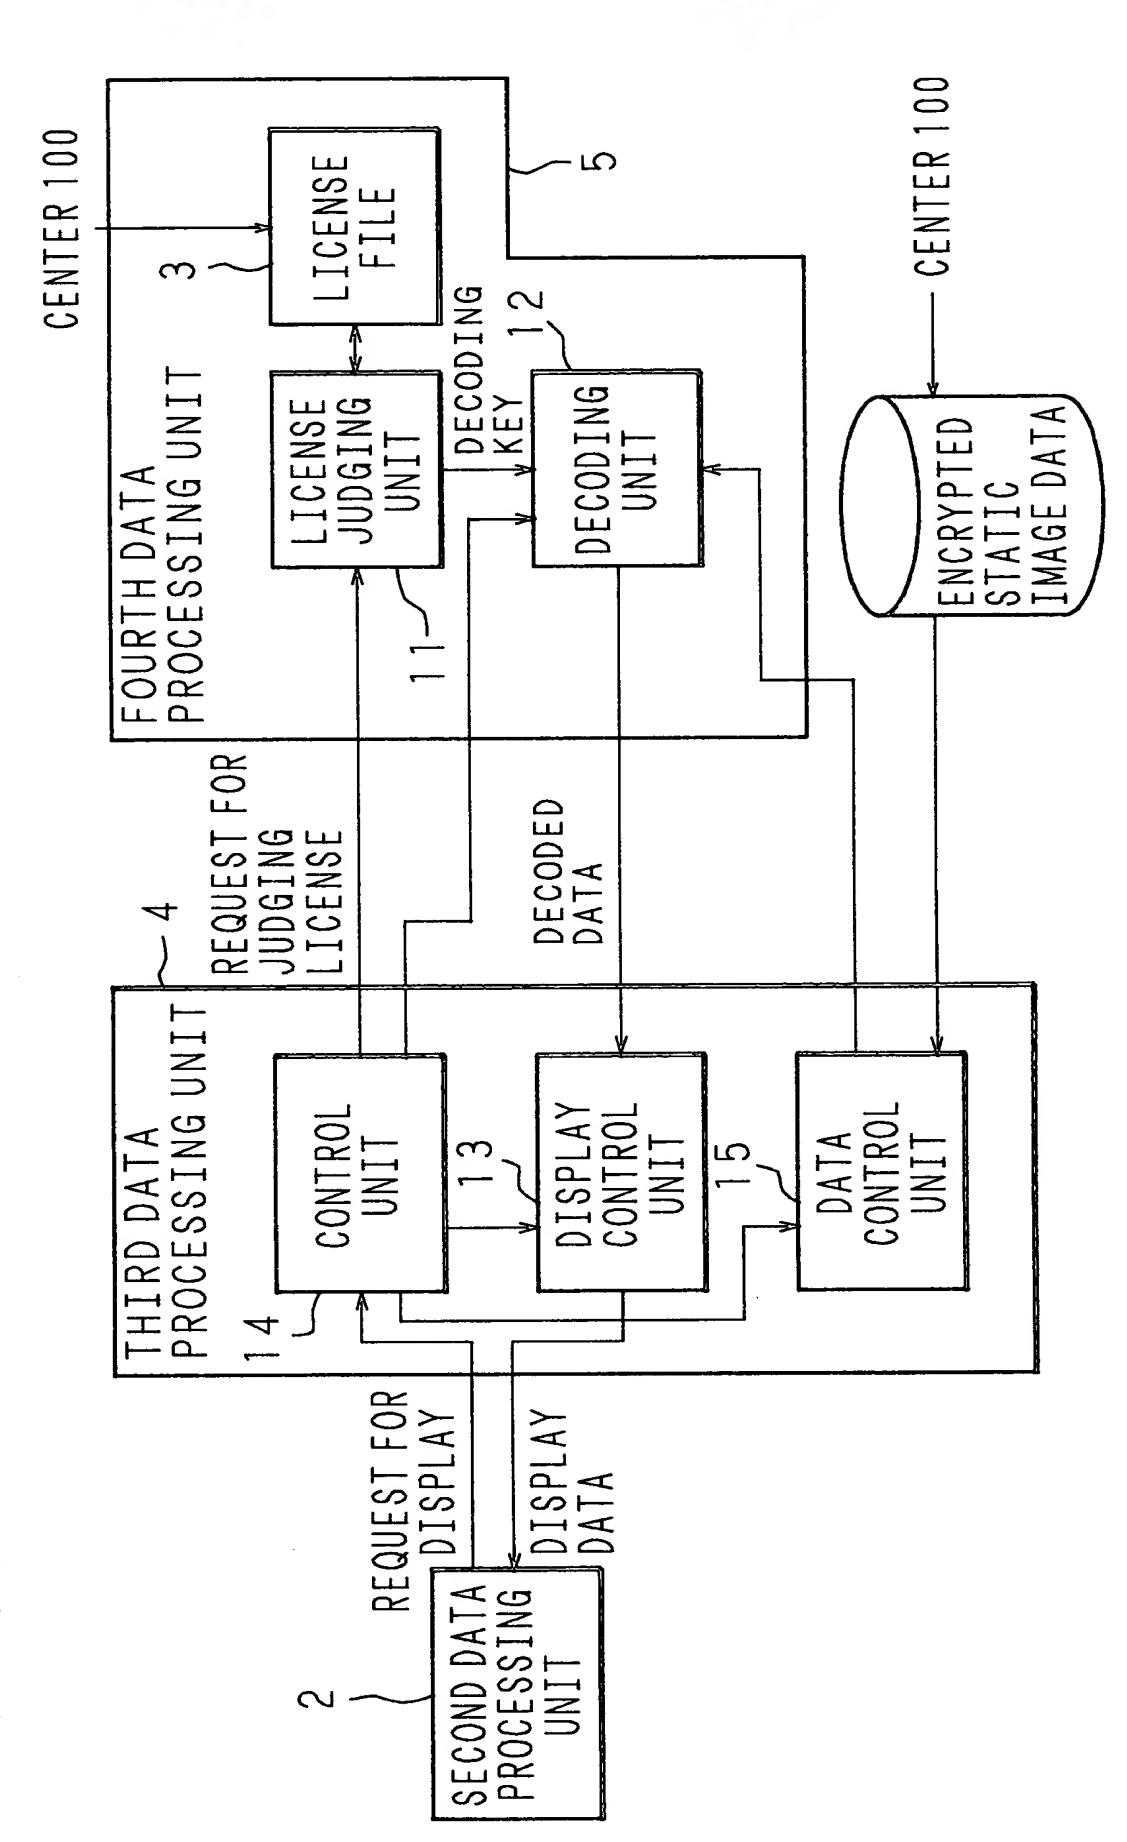
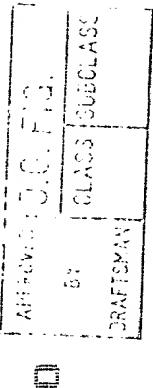


FIG. 8





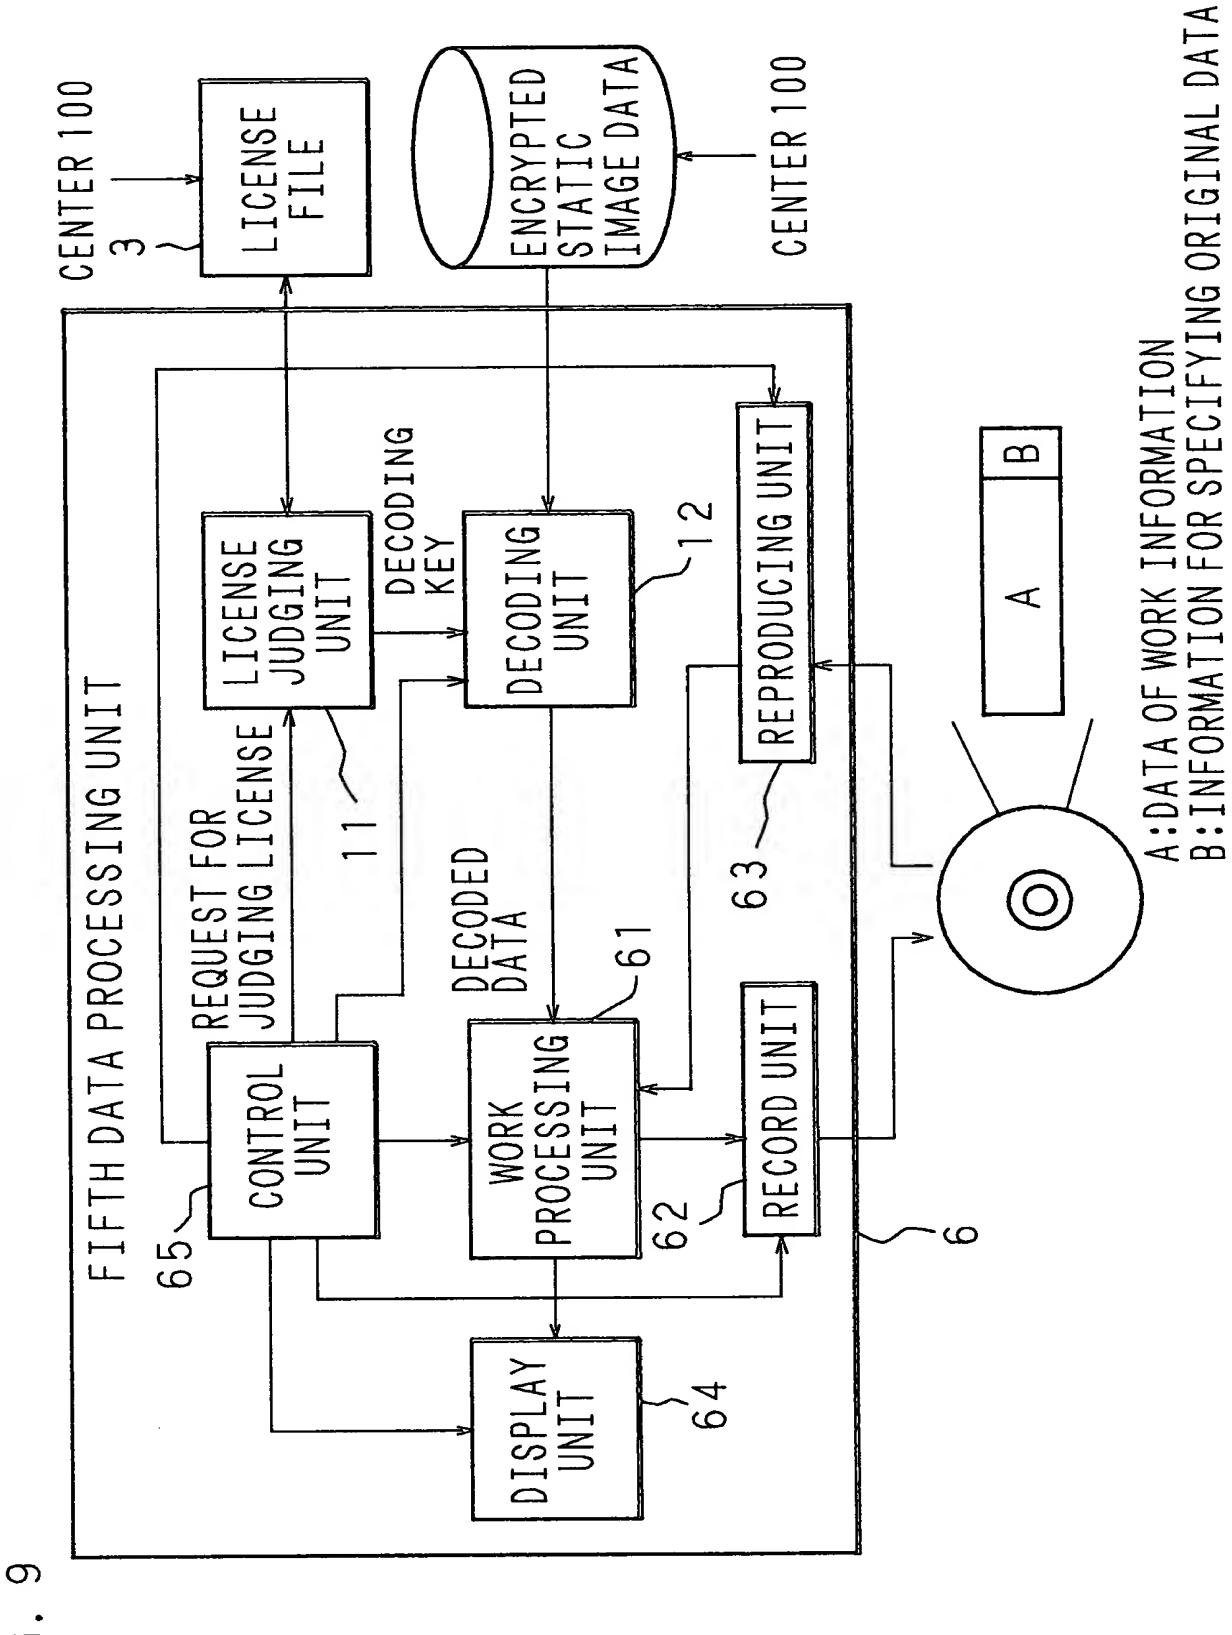



FIG.





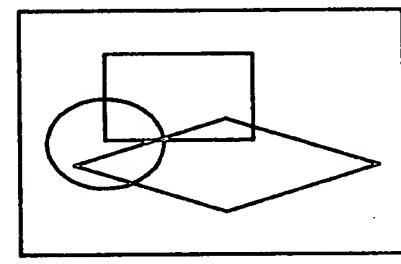


FIG. 10B

STATIC IMAGE AFTER WORK PROCESSING

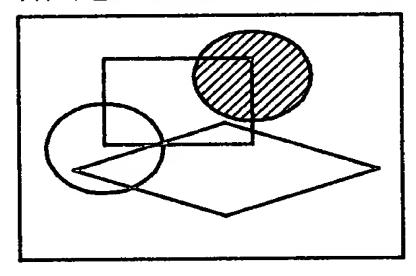
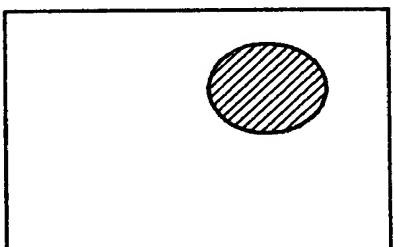


FIG. 10C

DIFFERENTIAL STATIC IMAGE (DATA OF WORK INFORMATION)



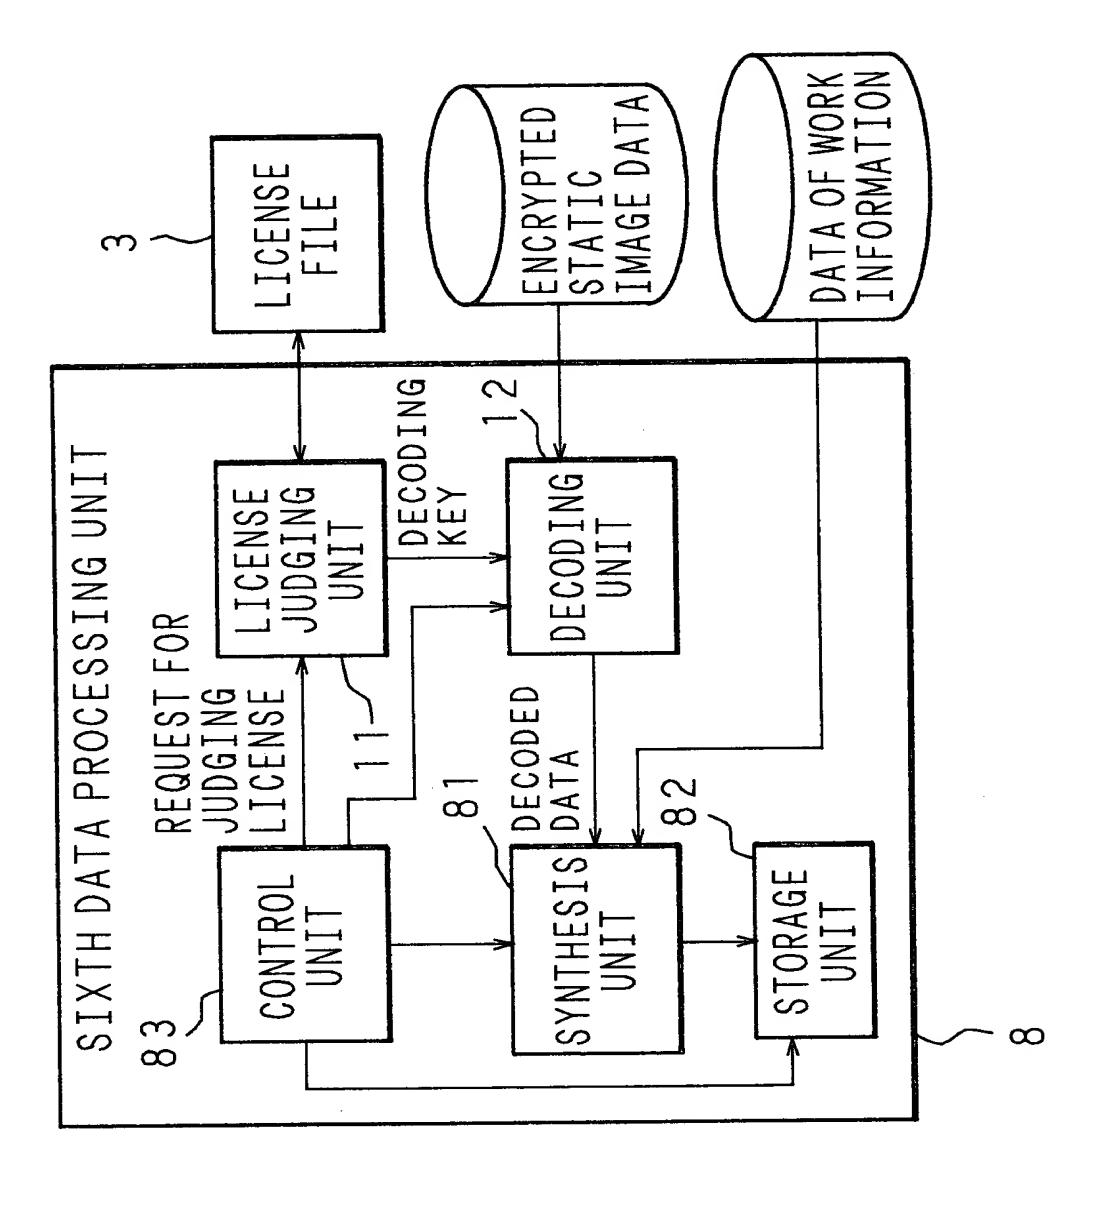


FIG. 1